

X-ray induced luminescence and spatial resolution of $\text{La}_2\text{O}_2\text{S:Tb}$ phosphor screens

I Kandarakis†, D Cavouras†, G Panayiotakis‡, T Agelis§, C Nomicos|| and G Giakoumakis||

† Department of Medical Instrumentation Technology, Technological Educational Institution of Athens, Athens, Greece

‡ Medical Physics Laboratory, School of Health Sciences, University of Patras, 265 00 Patras, Greece

§ Applied Physics Laboratory, Physics Department, University of Ioannina, 451 10 Ioannina, Greece

|| Department of Physics, Technological Educational Institution of Piraeus, Thivon, Aigaleo, Greece

Received 12 June 1995, in final form 23 October 1995

Abstract. Absolute efficiency and modulation transfer function of laboratory prepared $\text{La}_2\text{O}_2\text{S:Tb}$ phosphor screens of various coating thickness were studied. Detailed experimental data on the variation of absolute efficiency with x-ray tube voltage up to 200 kVp and screen coating thickness in transmission and reflection observation mode are given. Data were compared with similar results from other rare earth phosphor materials. Theoretical calculations were in good agreement with experimental data to permit estimation of intrinsic efficiency and coefficients related to light scattering and absorption within the phosphor material. The MTF of $\text{La}_2\text{O}_2\text{S:Tb}$ screens was also experimentally and theoretically evaluated.

1. Introduction

The efficiency and spatial resolution of various phosphor screens employed in medical image detectors are important parameters that affect image quality and radiation dose to the patient. Efficiency relative to other phosphor screens (Stevens and Schrama-de Pauw 1976, Sklensky *et al* 1974) as well as conversion efficiency, cathodoluminescent efficiency, quantum efficiency, scintillation efficiency, detective quantum efficiency, and luminance efficiency have been studied in a large number of papers (Wang *et al* 1970, Wickersheim *et al* 1970, Alig and Bloom 1977, Swank 1973, 1974, Bunch *et al* 1987, Nishikawa and Yaffe 1990, Beutel *et al* 1993, Ginzburg and Dick 1993, Wowk *et al* 1994). However, the absolute efficiency of screens under fluoroscopy conditions, defined as the ratio of light flux ϕ emitted towards the observation side divided by the incident x-ray beam power $N(n = \phi/N)$, is of value to people dealing with x-ray intensifying screens and image intensifiers (Nomicos *et al* 1978, Giakoumakis and Nomicos 1985, Giakoumakis *et al* 1989, 1990, 1993).

In the present work a systematic study of the absolute efficiency of laboratory prepared $\text{La}_2\text{O}_2\text{S:Tb}$ screens of various phosphor coating thicknesses was performed using x-ray tube voltages up to 200 kVp. Since radiographic screens are excited to luminescence in transmission and/or reflection modes of observation (i.e. the x-ray beam is incident on one side of the screen and light is detected at the opposite or the same side of the screen

respectively), both modes of observation were employed for the purposes of the present study. Also the MTF of those $\text{La}_2\text{O}_2\text{S:Tb}$ screens was studied in the transmission mode of observation, employing the square wave response function (SWRF) method (ICRU 1986) on digitized radiographic images. Experimental data were compared with corresponding theoretical models (Hamaker 1947, Ludwig 1971, Swank 1973, Beutel *et al* 1993).

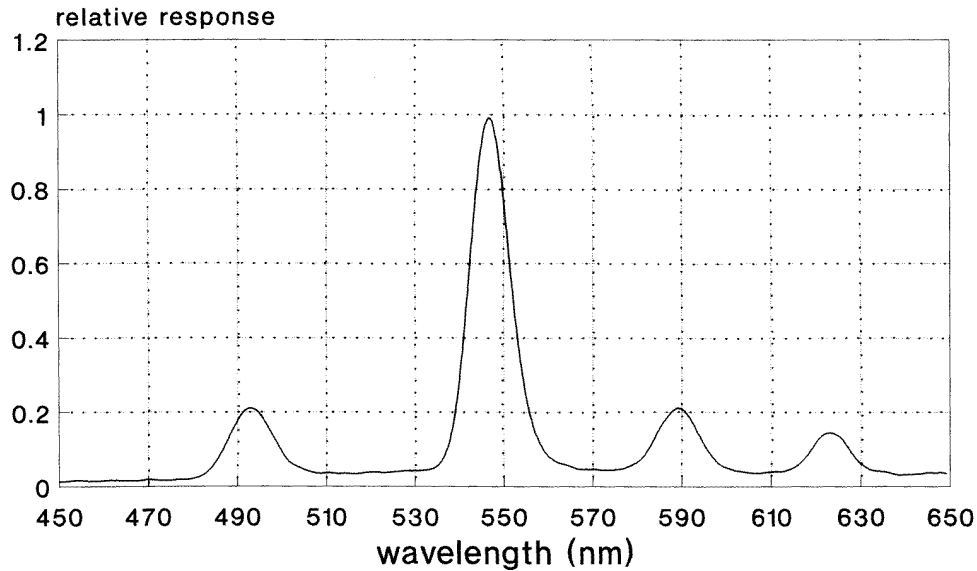


Figure 1. The spectral response of the $\text{La}_2\text{O}_2\text{S:Tb}$ screen.

2. Materials and methods

$\text{La}_2\text{O}_2\text{S:Tb}$ screens were prepared by sedimentation on fused silica substrates as described in previous studies for other phosphor materials (Giakoumakis *et al* 1990, 1993). Screen coating thickness varied between 13.6 mg cm^{-2} and 162 mg cm^{-2} . Screens outside that range were not used because they had extremely low efficiency or poor spatial resolution for radiography. The phosphor material was supplied in powder form by Derby Luminescents Ltd (code No LT133) with a mean grain size of $7 \mu\text{m}$.

The experimental set-up adopted for absolute efficiency measurements, comprising a Siemens Stabilipan x-ray unit and a photomultiplier tube with an extended sensitivity S-20 photocathode, has been analytically described in previous papers (Giakoumakis *et al* 1989, 1993). Screens were measured under fluoroscopy conditions in both transmission and reflection modes of observation. For each screen the variation of absolute efficiency with tube voltage was examined between 50 kVp and 200 kVp. The tube current was kept constant at 10 mA.

Absolute efficiency was calculated from the experimental data by taking into account (i) the ratio of light flux collected by the photocathode to the total light flux emitted by the screen towards the observation side and (ii) the matching factor between the spectral sensitivity of the S-20 photocathode and the $\text{La}_2\text{O}_2\text{S:Tb}$ phosphor spectrum. The latter was measured with an Oriel 7240 grating monochromator (figure 1) and the matching factor was calculated as described in a previous report (Giakoumakis 1991).

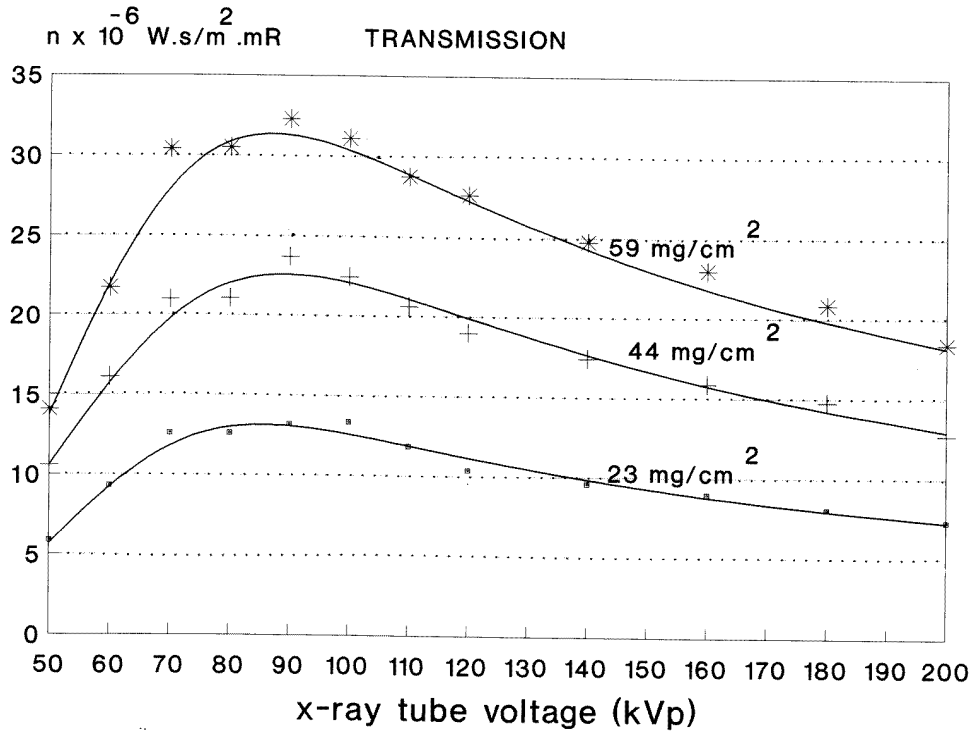


Figure 2. Absolute efficiency in transmission mode versus x-ray tube voltage for three La₂O₂S:Tb screens of 23, 44, and 59 mg cm⁻² coating thickness. Solid lines, theoretical results; points, experimental data.

Absolute efficiency was also calculated employing the theoretical model of Hamaker (1947) and Ludwig (1971). This model predicts the absolute efficiency of a phosphor screen excited by monochromatic x-rays by the following equations:

$$n_t = [n_c \gamma t \mu (1 + \rho) e^{(-\mu w)} / 2(\mu^2 - \sigma^2)] \times [(\mu - \sigma)(1 - \beta) e^{(-\sigma w)} + 2(\sigma + \mu\beta) e^{(\mu w)} - (\mu + \sigma)(1 + \beta) e^{(\sigma w)}] \times [(1 + \beta)(\rho + \beta) e^{(\sigma w)} - (1 - \beta)(\rho - \beta) e^{(-\sigma w)}]^{-1} \quad (1)$$

$$n_r = [n_c \gamma \mu e^{-\mu w} / (\mu^2 - \sigma^2)] \times [(\mu - \sigma)(\rho + \beta) e^{(\sigma w)} + 2(\sigma\rho - \mu\beta) e^{(-\mu w)} - (\mu + \sigma)(\rho - \beta) e^{(-\sigma w)}] \times [(1 + \beta)(\rho + \beta) e^{(\sigma w)} - (1 - \beta)(\rho - \beta) e^{(-\sigma w)}]^{-1} \quad (2)$$

where n_t and n_r are the absolute efficiencies in transmission and reflection modes respectively, n_c is the intrinsic efficiency of the phosphor, μ the mass attenuation coefficient for the incident x-ray photons, w the coating thickness (surface density) of the screen, t the transparency of the screen's substrate, $\rho = (1 - r)/(1 + r)$ where r is the reflectivity of the screen's substrate, γ is the conversion factor converting the energy fluence of the x-ray beam (W m^{-2}) to exposure rate (mR s^{-1}), and σ and β are coefficients directly related to the absorption (a) and scattering (s) coefficients of optical photons within the screen, by $\sigma = [a(a + 2s)]^{1/2}$ and $\beta = [a/(a + 2s)]^{1/2}$.

The spectral response of the x-ray tube and the absorption of the Al filter were also taken into account because the x-ray beam was polychromatic. Thus, the absolute efficiency

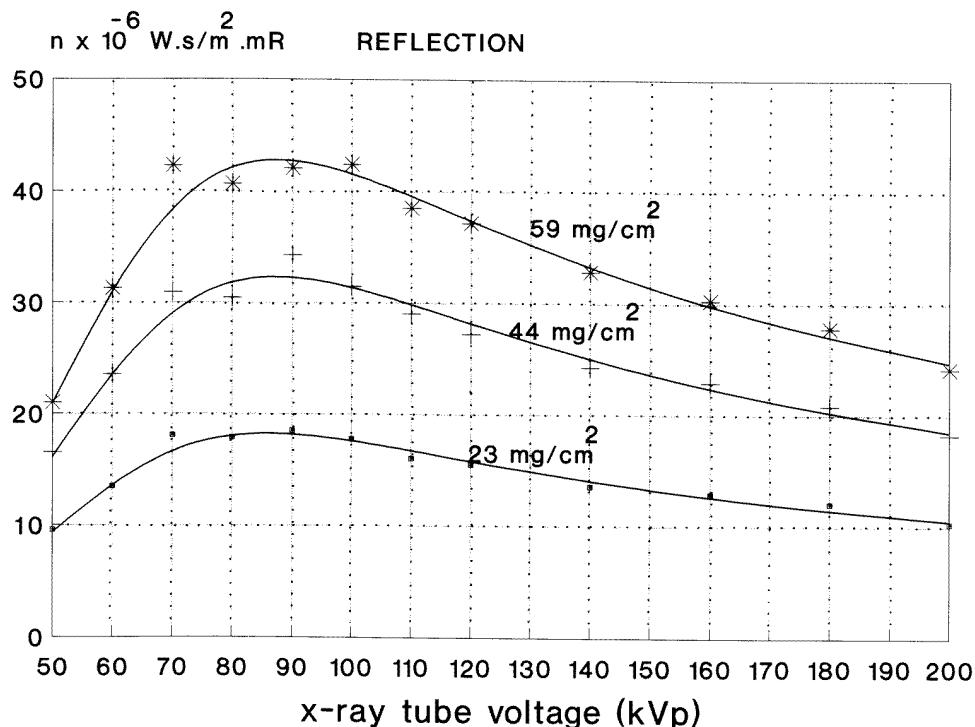


Figure 3. Absolute efficiency in reflection mode versus x-ray tube voltage for three $\text{La}_2\text{O}_2\text{S:Tb}$ screens of 23, 44, and 59 mg cm^{-2} coating thickness. Solid lines, theoretical results; points, experimental data.

was calculated by

$$n = \left(\int_0^{E_0} n(E) f(E) dE \right) / \int_0^{E_0} f(E) dE \quad (3)$$

where E_0 is the maximum energy of the x-ray photons determined by the tube voltage, $f(E)$ is the spectral distribution function of the x-ray beam, and $n(E)$ is the absolute efficiency of the screen for a monochromatic x-ray beam as given by relation (1) or (2). $f(E)$ is given by (Storm 1972)

$$f(E) = (1 - E/E_0) \exp(-\mu_{Al}d) \quad (4)$$

where d is the total Al filter thickness (22 mm, 2 mm tube filter + 20 mm Al employed to simulate x-ray attenuation by human tissue) and μ_{Al} is the aluminum x-ray attenuation coefficient.

The intrinsic efficiency n_c and coefficient σ of $\text{La}_2\text{O}_2\text{S:Tb}$ phosphor were estimated by fitting relation (3) to the absolute efficiency experimental data. Values for μ in formulae (1) and (2) were calculated from data on lanthanum, oxygen, and sulphur (Storm and Israel 1967, Saloman *et al* 1988). Coefficient β was calculated from reflectivity measurements performed as described by Ludwig (1971).

The MTF of the $\text{La}_2\text{O}_2\text{S:Tb}$ screens was measured using the SWRF method (ICRU 1986). The SWRFs were determined in transmission mode using a line-pair test pattern in contact with a screen-film combination; the latter consisted of laboratory prepared

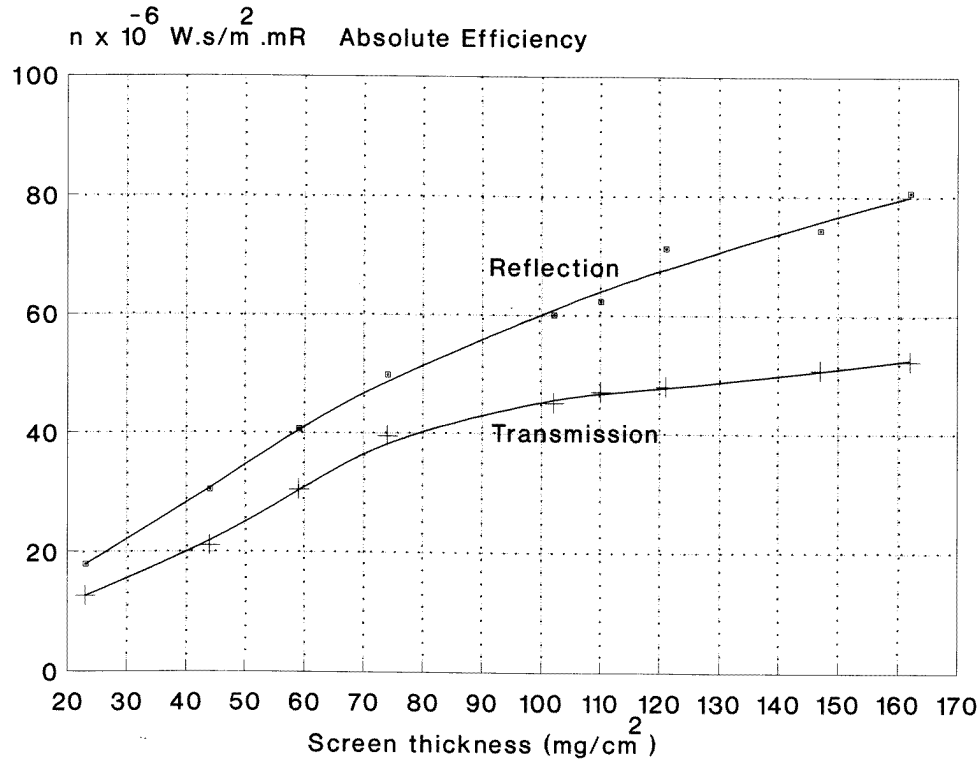


Figure 4. Absolute efficiency of La₂O₂S:Tb screens versus screen's coating thickness for both reflection and transmission mode, for 80 kVp x-ray tube voltage. Solid lines, theoretical results; points, experimental data.

La₂O₂S:Tb screens and Agfa Curix EA0449 radiographic films. The test pattern used (type 1-83) was made of lead with a nominal thickness of 0.05 mm and comprised line pairs of 17 spatial frequencies ranging between 0.5 lp cm⁻¹ and 50 lp cm⁻¹. Images of that test-pattern-screen system obtained on the radiographic films using a Phillips diagnostic x-ray unit at 80 kVp were transferred to a computer by means of a 470 000 pixel CCD camera and a frame grabber (Screen Machine II 512 × 512 × 8). For each screen the SWRF density pattern (pixel values) was computed from the screen's digital image as the mean of a large number of density patterns along parallel lines drawn vertically to the test-pattern line pairs, in order to eliminate noise. The SWRF patterns were normalized to the image contrast of the lowest spatial frequency, 0.5 lp cm⁻¹, as described in a previous report by Hillen *et al* (1987). The MTF was then calculated employing the following relation:

$$\text{MTF}(f) = (\pi/4)[\text{SWRF}(f)/1 + \text{SWRF}(3f)/3 - \text{SWRF}(5f)/5 + \text{SWRF}(7f)/7 - \dots]. \quad (5)$$

However, the MTF calculated in (5) is the combined effect of the video acquisition system MTF and screen MTF (film MTF ≈ 1 for frequencies ≤ 10 mm⁻¹ (Beutel *et al* 1993)). Thus La₂O₂S:Tb screen MTF was determined as follows:

$$\text{MTF}_{\text{La}_2\text{O}_2\text{S:Tb}} = \text{MTF}_{\text{com}}/\text{MTF}_{\text{VAS}} \quad (6)$$

where MTF_{com} is the combined system MTF including screen, calculated in (5), and MTF_{VAS}

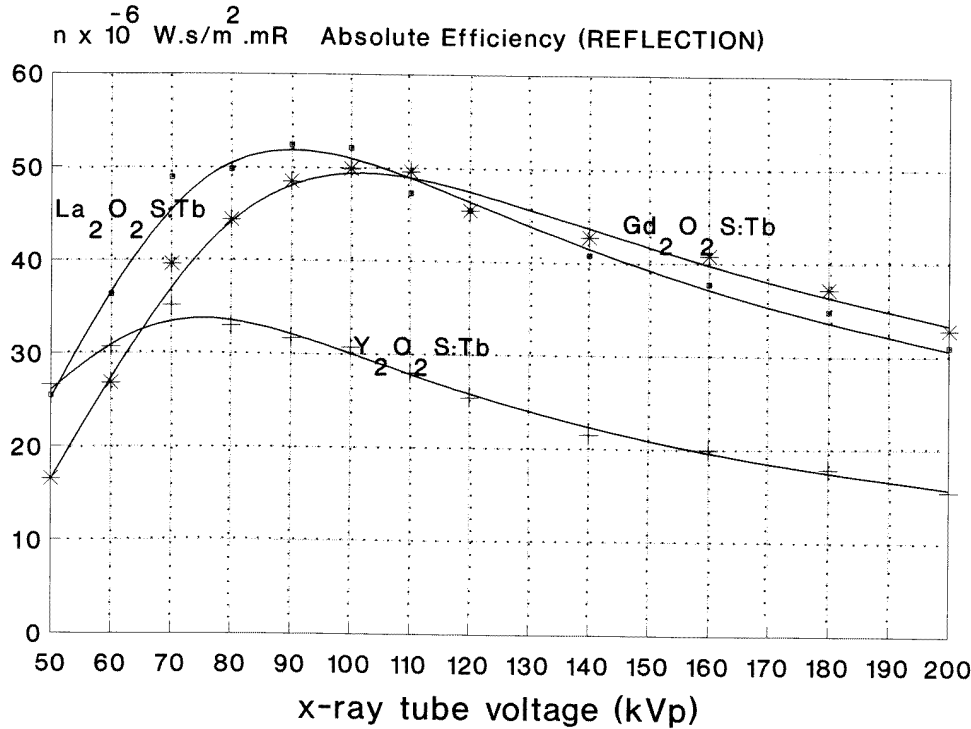


Figure 5. The variation of absolute efficiency measured in reflection mode for $Y_2O_2S:Tb$, $La_2O_2S:Tb$ and $Gd_2O_2S:Tb$ screens of approximately the same coating thickness (70 mg cm^{-2}). Solid lines, theoretical results; points, experimental data.

is the MTF of the video acquisition system. The latter was determined from images captured with the test pattern mounted on the light box. The linearity of the video acquisition system was verified by digitizing a step wedge radiographic image of known optical densities (Doler *et al* 1994). Additionally, the MTF was theoretically calculated using Swank's model equations (Swank 1973):

$$\begin{aligned}
 \text{MTF}(E, f) = & \mu\tau\rho_1 e^{-\mu w} \\
 & \times [2q(\tau\rho_0 + \mu) e^{-\mu w} - (\mu + q)(q + \tau\rho_0) e^{qw} - (\mu - q)(q - \tau\rho_0) e^{-qw}] \\
 & \times \{(1 - e^{-\mu w})(\mu^2 - q^2)[(q + \tau\rho_0)(q + \tau\rho_1) e^{qw} \\
 & - (q - \tau\rho_0)(q - \tau\rho_1) e^{-qw}]\}^{-1}
 \end{aligned} \quad (7)$$

where $q = (4\pi^2 f^2 + \sigma^2)^{1/2}$, $\tau = \sigma/\beta$, $\rho_0 = (1 - r_0)/(1 + r_0)$, $\rho_1 = (1 - r_1)/(1 + r_1)$, where r_0 is the reflectivity of the screen-film interface and r_1 the reflectivity of the screen-substrate interface. μ , σ , β and w are defined in equations (1) and (2).

Since equation (7) holds for monoenergetic x-rays an integration over the x-ray spectrum was performed as follows:

$$\text{MTF}(f) = \left(\int_0^{E_0} \text{MTF}(E, f) f(E) dE \right) / \int_0^{E_0} \text{MTF}(E, 0) f(E) dE. \quad (8)$$

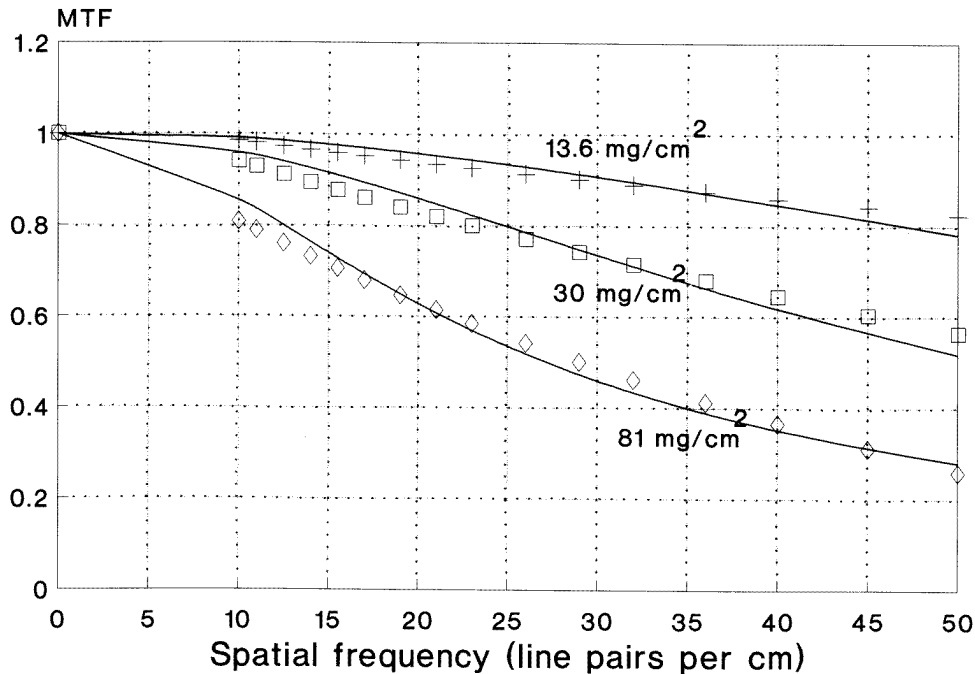


Figure 6. MTF curves for three La₂O₂S:Tb screens of 13.6, 30, and 81 mg cm⁻² coating thickness. Solid lines, calculated MTF values; points, experimental data.

3. Results and discussion

In figures 2 and 3 the variation of absolute efficiency with tube voltage is presented in transmission and reflection mode respectively for three screens of different thickness. Peak efficiency was in the range between 70–90 kVp, depending on screen thickness. In figure 4 efficiency at 80 kVp is plotted against coating thickness, both in transmission and in reflection mode. Screens in reflection mode were more efficient than in transmission mode, because in the latter light photons travel longer distances to reach the emitting screen surface. Solid lines in figures 2–4 represent the best fitted curves through the experimental data achieved employing relations (1)–(3), giving $\sigma = 30 \text{ cm}^2 \text{ g}^{-1}$ and $n_c = 0.18$; the latter is higher than values reported previously for cathodoluminescence efficiency (Wickersheim *et al* 1970, Alig and Bloom 1977). Coefficient β , found by reflectivity measurements, was equal to 0.03. The variation of absolute efficiency with tube voltage for three phosphor materials (Y₂O₂S:Tb, La₂O₂S:Tb, and Gd₂O₂S:Tb) with approximately the same coating thickness (70 mg cm⁻²) is presented in figure 5. Data for Gd₂O₂S:Tb and Y₂O₂S:Tb phosphors were obtained using the same experimental set-up and theoretical calculations as for La₂O₂S:Tb (Giakoumakis and Nomicos 1985, Giakoumakis *et al* 1989, 1990). Gd₂O₂S:Tb screens are more efficient at higher and La₂O₂S:Tb screens are better at lower and intermediate tube voltages. It is interesting to note that Y₂O₂S:Tb is more efficient than Gd₂O₂S:Tb at relatively low kVp (lower than 65 kVp for data shown in figure 5) and it also seems to be more efficient than La₂O₂S:Tb at even lower voltages (lower than 50 kVp in figure 5). The peak efficiency value of La₂O₂S:Tb obtained at 90 kVp is higher than that of Gd₂O₂S:Tb obtained at 100–110 kVp. Differences in absolute efficiency may be attributed

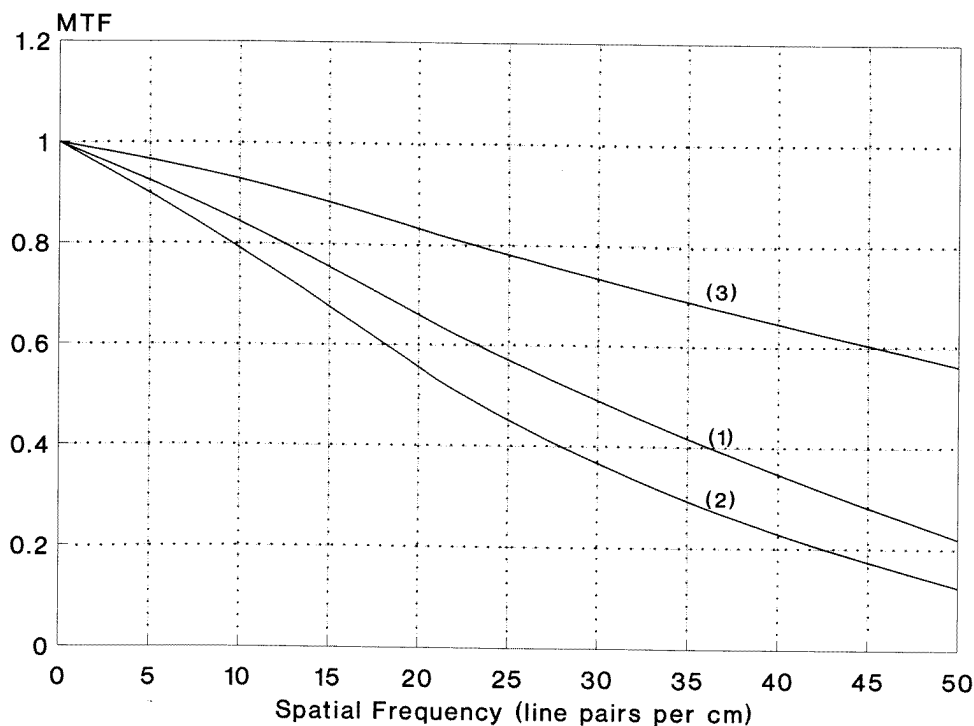


Figure 7. The MTF curve of the video acquisition system (1) and the measured (2) and corrected (3) MTF curves of a 30 mg cm^{-2} $\text{La}_2\text{O}_2\text{S:Tb}$ phosphor screen.

mainly to differences in x-ray attenuation coefficients (K-edge absorption energies) among phosphor materials, since deviations in σ , β , and n_c (table 1) were insignificant.

Table 1. Optical data for the three phosphors.

	n_c^a	σ^b ($\text{cm}^2 \text{ g}^{-1}$)	β^b
$\text{Y}_2\text{O}_2\text{S:Tb}$	0.18	30	0.03
$\text{La}_2\text{O}_2\text{S:Tb}$	0.18	30	0.03
$\text{Gd}_2\text{O}_2\text{S:Tb}$	0.20	30	0.03

^a Intrinsic efficiency of the phosphor.

^b Coefficients directly related to the absorption and scattering coefficients of optical photons within the screen.

The variation of MTF with spatial frequency for $\text{La}_2\text{O}_2\text{S:Tb}$ screens of different thicknesses is shown in figure 6. Solid lines represent theoretical results obtained by relations (7) and (8) and dots experimentally determined MTF data. In figure 7, curve 2 shows the combined effect of the MTF of a 30 mg cm^{-2} screen and the MTF of the video acquisition system; curve 2 was obtained using Coltman's formula (relation (5)) and performing SWRF measurements. As observed, the combined MTF of the screen decreases to 0.13 at the limiting frequency of 50 lp cm^{-1} . Curve 1 is the MTF of the video acquisition system, also obtained employing relation (5) on the digitized image of the test pattern alone. After experimental determination of curves 1 and 2, it was possible to derive

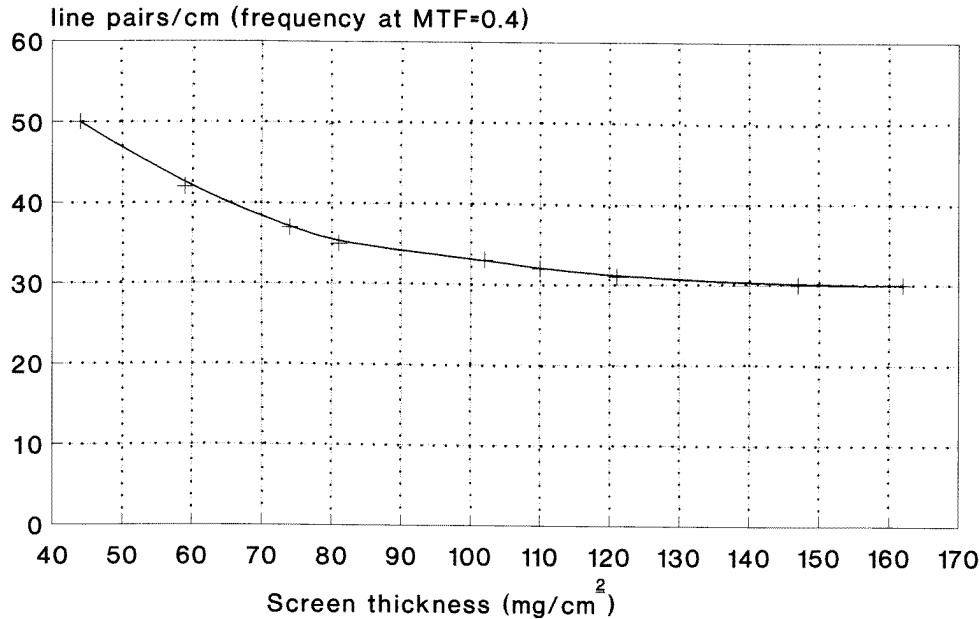


Figure 8. Calculated values of resolution (frequency at MTF = 0.4) against screen coating thickness for La₂O₂S:Tb screens.

the MTF of the 30 mg cm⁻² La₂O₂S:Tb screen using relation (6). As it can be deduced from figures 6 and 7, the resulting correction provides curves in good approximation to the curves which were theoretically obtained by Swank's model (relations (7) and (8)). The agreement between theoretically and experimentally determined MTF curves is indicative of the validity of the method employed in the present study. The video acquisition system can provide reliable results for frequencies up to 50 lp cm⁻¹ and for thicknesses from about 10 to 110 mg cm⁻², which is the thickness range of many commercial radiographic screens. For thicker screens, MTF measurements were difficult to obtain at high frequencies due to inherent resolution limitations of the CCD camera-frame grabber system. Therefore, the variation of the screen resolution with coating thickness was assessed at MTF = 0.4. The curve of figure 8 has a hyperbolic behaviour, indicating that for screen thicknesses over 120 mg cm⁻² the decrease in resolution is insignificant. Despite the frequency limitations, the CCD camera-frame grabber system is fast and easily accessible at user level. Similar set-ups, employing a camera interfaced to a computer, have been successfully applied in evaluating the Wiener spectrum of TV viewed fluoroscopic systems (Goldman 1992) and the MTF of on-line portal imaging screens in radiation therapy (Wowk *et al* 1994). However, the microdensitometer, although expensive and cumbersome to use, is more appropriate for applications demanding higher accuracy, especially at high frequencies (Dainty and Shaw 1974, Barnes 1979, Cunningham and Reid 1992).

4. Summary and conclusions

The absolute efficiency and spatial resolution of La₂O₂S:Tb screens were studied. The intrinsic efficiency and coefficients related to scattering and absorption of light photons

within the screens were also found using a uniform screen theoretical model. The intrinsic efficiency of the $\text{La}_2\text{O}_2\text{S:Tb}$ screens was found to be equal to that of $\text{Y}_2\text{O}_2\text{S:Tb}$ and slightly lower than that of $\text{Gd}_2\text{O}_2\text{S:Tb}$. Light absorption and scattering was about the same for all three phosphors. The $\text{La}_2\text{O}_2\text{S:Tb}$ absolute efficiency was higher in the lower and intermediate kVp range and $\text{Y}_2\text{O}_2\text{S:Tb}$ seemed better in the very low kVp range. Screen MTF determination by CCD camera interfaced to a computer is fast and could be applied routinely.

References

- Alig R C and Bloom S 1977 Cathodoluminescence efficiency *J. Electrochem. Soc.* **124** 1136–8
- Barnes G T 1979 The use of bar pattern test objects in assessing the resolution of film/screen systems *The Physics of Medical Imaging: Recording System Measurements and Techniques* ed A G Haus (New York: American Association of Physicists in Medicine) pp 138–51
- Beutel J, Apple B A and Shaw R 1993 The role of screen parameters and print-through in the performance of film/screen systems *Phys. Med. Biol.* **38** 1181–206
- Bunch P C, Huff K E and Van Metter R 1987 Analysis of the detective quantum efficiency of a radiographic film–screen combination *J. Opt. Soc. Am. A* **4** 902–9
- Cunningham I A and Reid B K 1992 Signal and noise in modulation transfer function determinations using slit, wire, and edge techniques *Med. Phys.* **19** 1037–44
- Dainty J C and Shaw R 1974 *Image Science* (New York: Academic)
- Doler W, Rassow St, Jager A and Vosshenrich R 1994 Investigation of the imaging properties of an x-ray film scanner *Phys. Med. Biol.* **39** 917–22
- Giakoumakis G E 1991 Matching factors for various light source–photodetector combinations *Appl. Phys. A* **52** 7–9
- Giakoumakis G E and Nomicos C D 1985 Absolute efficiency of $\text{Y}_2\text{O}_2\text{S:Tb}$ screens under fluoroscopy conditions *J. Appl. Phys.* **58** 2742–5
- Giakoumakis G E, Nomicos C D and Sandilos P X 1989 Absolute efficiency of $\text{Gd}_2\text{O}_2\text{S:Tb}$ screens under fluoroscopic conditions *Phys. Med. Biol.* **34** 673–8
- Giakoumakis G E, Nomicos C D, Skountzos P, Koutroubas S et al 1993 $\text{Y}_2\text{O}_2\text{S:Eu}$ phosphor screen evaluation *Med. Phys.* **20** 79–83
- Giakoumakis G E, Nomicos C D, Yiakoumakis E N and Evangelou E K 1990 Absolute efficiency of rare earth oxysulfide screens in reflection mode observation *Phys. Med. Biol.* **35** 1017–23
- Ginzburg A and Dick C E 1993 Image information transfer properties of x-ray intensifying screens in the range from 17 to 320 keV *Med. Phys.* **20** 1013–21
- Goldman L W 1992 Fluoroscopic performance tests using a portable computer/frame grabber: Wiener spectra measurements *Med. Phys.* **19** 45–52
- Hamaker H 1947 Radiation and heat conduction in light-scattering material *Philips Res. Rep.* **2** 55–67
- Hillen W, Schiebel U and Zaengel T 1987 Imaging performance of a digital storage phosphor system *Med. Phys.* **14** 744–51
- ICRU 1986 MTF of screen–film systems *ICRU Report* 41
- Ludwig G W 1971 X-ray efficiency of powder phosphors *J. Electrochem. Soc.* **118** 1152–9
- Nishikawa R M and Yaffe M J 1990 Model of the spatial frequency dependent detective quantum efficiency of phosphor screens *Med. Phys.* **17** 894–904
- Nomicos C D, Giakoumakis G E, Euthymiou P C and Sandilos P X 1978 Absolute efficiency of ZnCdS:Ag phosphor under fluoroscopy conditions *J. Appl. Phys.* **49** 3636–8
- Saloman E B, Hubbell J H and Scofield J H 1988 X-ray attenuation cross-sections for energies 100 eV to 100 keV and elements $Z = 1$ to $Z = 92$ *At. Data Nucl. Data Tables* **38** 1–197
- Sklensky A F, Buchanan R A, Maple T G and Bailey H N 1974 Quantum utilization in x-ray intensifying screens *IEEE Trans. Nucl. Sci.* **NS-21** 685–91
- Stevens A L N and Schrama-de Pauw A D 1976 Theoretical and experimental efficiencies of x-ray screens *J. Electrochem. Soc.* **123** 886–8
- Storm E 1972 Calculated bremsstrahlung spectra from thick tungsten targets *Phys. Rev. A* **5** 2328–38
- Storm E and Israel H 1967 Photon cross-sections from 0.001 to 100 MeV for elements 1 through 100 *Los Alamos Scientific Laboratory of the University of California Report* LA-3753
- Swank R 1973 Calculation of Modulation Transfer Function of x-ray fluorescent screens *Appl. Opt.* **12** 1865–70

- Swank R 1974 Absorption and noise in x-ray phosphors *J. Appl. Phys.* **45** 4109–203
- Wang S P, Laudi O, Lucks H, Wickersheim K A and Buchanan R A 1970 X-ray image intensifier tubes using rare earth oxysulfide phosphors *IEEE Trans. Nucl. Sci.* **NS-17** 49–56
- Wickersheim K A, Alves R V and Buchanan R A 1970 Rare earth oxysulfide x-ray phosphors *IEEE Trans. Nucl. Sci.* **NS-17** 57–60
- Wolk B, Radcliffe T, Leszczynski K W, Shavel S and Rajapakshe R 1994 Optimization of metal phosphor screens for on-line portal imaging *Med. Phys.* **21** 227–35